

Accessories



CHIROBLOC Ballast - ref. CBL

It is an independent spare part made out of stainless steel, it may be attached to CHIROBLOC to weigh it.

Weight: 0.780kg

5 years warranty.



RING - ref. RING

RING will be used as an attachment to any CHIROBLOC.

Sold separately by box of 10 units.

Warranty: 1 year

RING will replace rubber bands made from surgical gloves.



Design: e-moneaux.fr / 252 éd.05 - © AREX® - 2020

CHIROBLOC3 - ref. CHIRO3

Made out of a composite bio-compatible material.


Radio-lucency without lead weight.

Will not stain surgical gloves.

- One wrist band:
two possible adjustments

Wrist strap /
child positioning

Wrist strap /
adult positioning

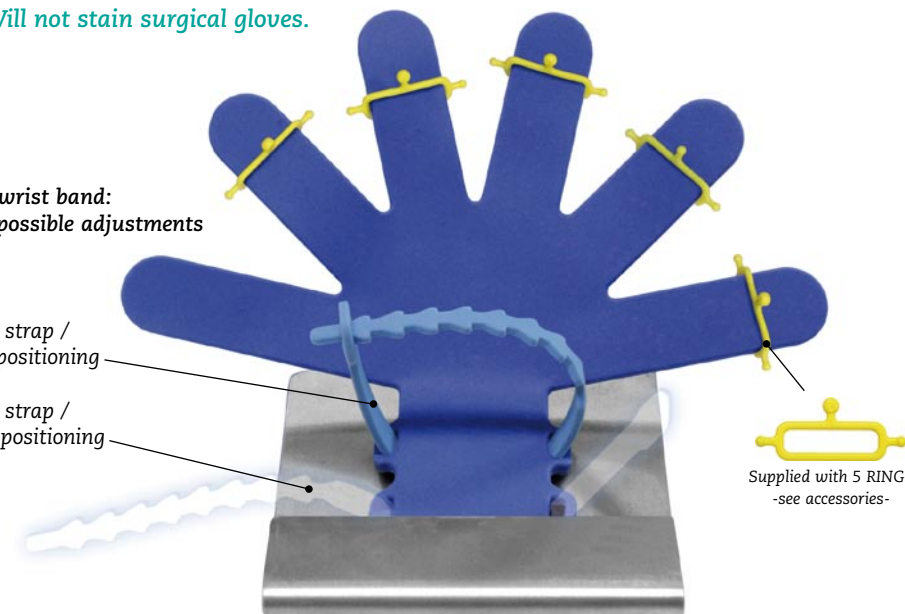

Supplied with 5 RINGS
-see accessories-


CHIROBLOC Ballast - see accessories

CHIROBLOC3

Supplied with 5 RINGS

Weight: 0.27kg

Warranty: 1 year

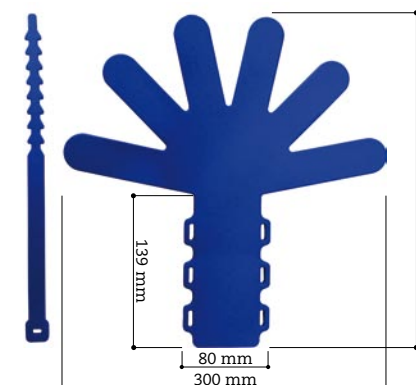


DISTRIBUTED BY



Manufacturer:
AREX®
3 allée du Clos Tonnerre
91120 Palaiseau - FRANCE

www.arex.fr

CHIROBLOC3 & Mini-open CTR

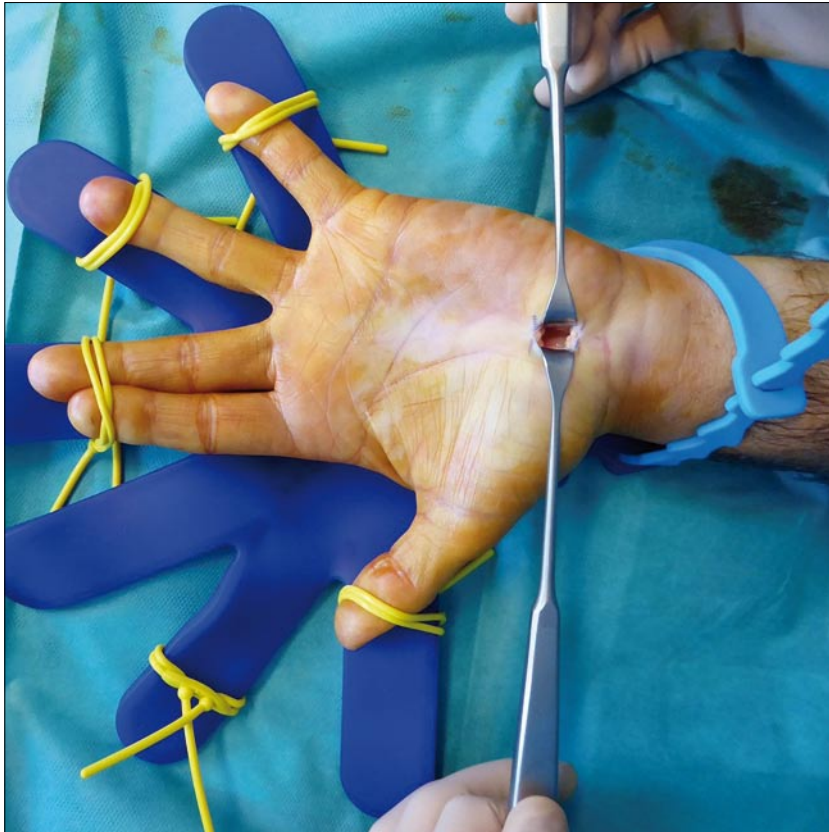

Philippe Liverneux MD - Strasbourg University Hospital - France

CHIROBLOC3 & Endoscopic CTR



Didier Fontes MD - Paris, Clinique du Sport - France